

# Application of self-absorption correction method in gamma spectroscopy for $^{210}\text{Pb}$ and $^{137}\text{Cs}$ sediment chronology on the continental slope off NW Africa

Daniela Pittauerová<sup>1</sup>, Stefan Mulitza<sup>2</sup>, Bernd Hettwig<sup>1</sup>, Wissam Chehade<sup>1</sup>, Gesine Mollenhauer<sup>2</sup>, Jan-Berend Stuut<sup>2</sup>, Helmut W. Fischer<sup>1</sup>

<sup>1</sup> University of Bremen, Department of Physics, Radioactivity Measurements Laboratory, Otto-Hahn-Allee 1, D-28334 Bremen, Germany. <sup>2</sup> University of Bremen, MARUM, Leobener Strasse, D-28359 Bremen, Germany

## INTRODUCTION

### Climatological background

Life in the semiarid Sahel belt of tropical North Africa strongly depends on the availability of water and has been repeatedly affected by shifts to more arid climate. The most recent drought occurred in the early 1970's and 1980's, with partial recovery during the late 1990's. High resolution fluvial sediments off Senegal offer the opportunity to study the history of the Sahel drought and to assess its imprint on the composition of terrestrial materials deposited at the sea floor, if the material can be accurately dated on historical time scales.

### Sediment chronology

With the background of the upper mentioned project, we present  $^{210}\text{Pb}$  and  $^{137}\text{Cs}$  data from the high resolution multi-core GeoB9501-4 recovered during METEOR-Cruise M65/1 on the continental slope off NW Africa (Senegal Mudbelt, northern rim of Mauritanian Canyon, depth 330 m). The uppermost 50 cm of the multi-core has been used for improving routine technique of  $^{210}\text{Pb}$  and  $^{137}\text{Cs}$  sediment chronology in the Radioactivity Measurement Laboratory of Bremen University.

### Self attenuation

Since attenuation of emitted low-energy gamma radiation in voluminous bulk samples is an obstruction for determining  $^{210}\text{Pb}$  (46.5 keV,  $I_\gamma$  4.25%) quantitatively by means of gamma-spectroscopy, self-absorption correction must be taken into account. Two basic approaches have been applied for solving the problem of self-attenuation in volume samples: experimental (Cutshall *et al.*, 1983, San Miguel *et al.*, 2002) and mathematical – using Monte Carlo simulations (Sima and Dovlete, 1997). The approach combining both experimental measurements and mathematical MC simulations was proposed by García-Talavera and Peña (2004) and Hurtado *et al.* (2007).

## METHODS

### Gamma spectroscopy

A coaxial HPGe detector Canberra Industries (50% rel. efficiency) housed in a 10 cm Pb shielding with Cu and plastic lining operated under Genie 2000 software was used for low level, low-background gamma spectroscopy. The method used by authors in this study to deal with self attenuation is applying efficiencies calculated using LabSOCS<sup>TM</sup> (Laboratory SOurceless Calibration System), Genie 2000 software calibration tool (Bronson, 2003),

validated by self-absorption measurements of different materials.

### Material test

To validate the efficiency calibration generated by LabSOCS, a transmission experiment was realized for different absorbers. As emitters, point sources of gamma energies of 46.5 keV ( $^{210}\text{Pb}$ ) and 661.6 keV ( $^{137}\text{Cs}$ ) with reported activities (produced by Buchler) were used on a holder 15 cm above the absorber, which was placed directly on the detector (Fig. 1). Five different materials with various chemical composition and densities were used as absorbers, all of them sealed in cylindrical plastic containers (round dishes) with diameter of 70 mm and height of 20 mm (the same containers were used for sediment samples): air (density  $0\text{ g}\cdot\text{cm}^{-3}$ ), water (density  $1\text{ g}\cdot\text{cm}^{-3}$ ), wax (composition: 15% H and 85% C, density  $0,96\text{ g}\cdot\text{cm}^{-3}$ ), sea sand (composition: 50% quartz, 50% K-feldspar, bulk density  $1,4\text{ g}\cdot\text{cm}^{-3}$ ) and milled limestone (composition:  $\text{CaCO}_3$ , bulk density  $1,77\text{ g}\cdot\text{cm}^{-3}$ ). The sample geometry modelling and efficiency calibration file generation were performed using the Geometry Composer feature of the Genie 2000 software. The efficiency for given energies are estimated by LabSOCS for characterized detector based on MCNP modelling code upon description of a sample container, absorber matrix, and a specific source-to-detector distance.

The efficiencies were used for analyzing gamma-spectra of the point sources using experimental setup with above listed absorbers and estimating their activities using software Genie 2000. The gamma spectra of absorbers were collected separately and were subtracted from spectra of transmission experiments. The calculated activities of point sources were compared to their reported activities (Fig. 2). The experiment showed that activities estimated using LabSOCS generated efficiencies are within the overall error produced by Genie2000. It is planned to apply the same setup for direct determination of the sample's self absorption. Measurements in this respect are under way.



Fig. 1: Experiment setup

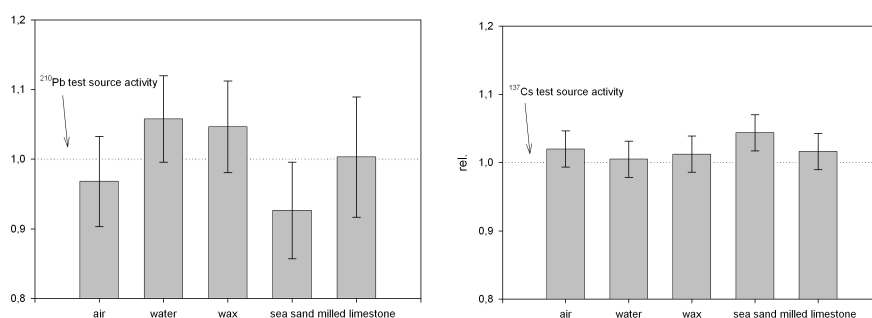


Fig. 2: Real relative activities of a  $^{210}\text{Pb}$  (left) and a  $^{137}\text{Cs}$  (right) point gamma test sources compared to activities estimated by measurement of their activities using absorbers of different chemical compositions and densities. The efficiencies were generated by LabSOCS.

### Measurement of sediment samples

Wet sediment slices from each 1 cm interval of multi-core GeoB9501-4 were put into plastic round dishes with diameter of 70 mm and height of 20 mm, the containers were filled with the samples into different heights. For determination of  $^{210}\text{Pb}_{\text{exc.}}$  activity,  $^{210}\text{Pb}_{\text{sup.}}$  activity (determined via the 351.9 keV line of  $^{214}\text{Pb}$  after establishing of Rn progeny equilibration)

was subtracted from the  $^{210}\text{Pb}_{\text{total}}$  signal. The spectra were analyzed using efficiencies generated by LabSOCS for different sample geometries and constant sediment composition.

### $^{210}\text{Pb}$ and $^{137}\text{Cs}$ dating

The age of the core has been estimated by  $^{210}\text{Pb}$  chronology using CRS model (Appleby and Oldfield, 1978). The model assumes a constant rate of supply of unsupported  $^{210}\text{Pb}$  to the sediment per unit time and considers a variable sedimentation rate resulting from human activity. Absolute ages were calculated with assumption the uppermost slice of the core corresponds to 2005 AD.  $^{137}\text{Cs}$  is present in the sediments due to the global fallout after nuclear bomb testing. It first appeared in the atmosphere in 1945 and peaked in 1963 at the northern hemisphere and can be therefore used for additional calibration of the age.

## RESULTS AND CONCLUSIONS

Volume activities of  $^{210}\text{Pb}_{\text{unsupported}}$  vs depth and volume activities of  $^{137}\text{Cs}$  decay corrected to the relevant age vs age are shown in the Fig. 3.

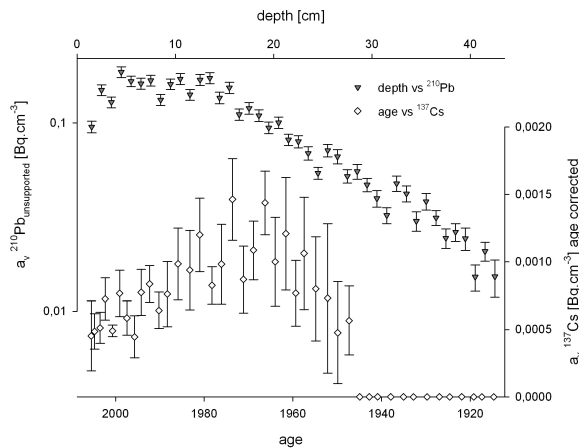


Fig. 3:  $^{210}\text{Pb}$  and  $^{137}\text{Cs}$  data of gravity core GeoB9501-4

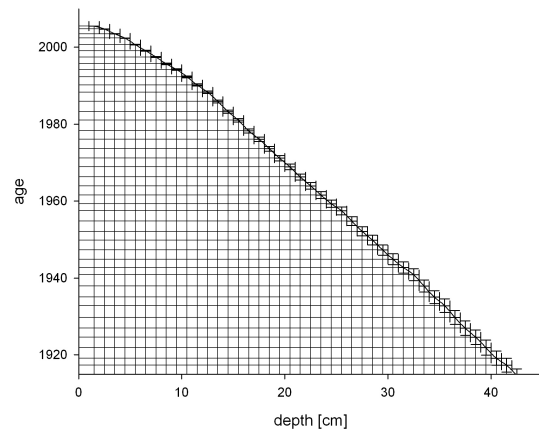


Fig. 4: Sedimentation rate estimated from the  $^{210}\text{Pb}_{\text{exc.}}$  using CRS chronology model

According to the ANNEX C of the UNSCEAR report (UNSCEAR, 2002), the total amount of  $^{137}\text{Cs}$  deposited from 1945 to 2000 in latitudinal band of 10-20 degrees north recalculated to 2007 activities (time of the measurement) is  $660 \text{ Bq}\cdot\text{m}^{-2}$ . Comparing the total activity of  $150 \text{ Bq}\cdot\text{m}^{-2}$  found in the core GeoB9501-4 to the UNSCEAR value, only 23% of expected value was preserved in the sediment record. Due to rather low  $^{137}\text{Cs}$  values the measurement errors are relatively high and do not provide fine resolution (expected 1963 peak or contribution of geographically close 4 Algerian atmospheric tests in 1960-61). Nevertheless, the shape of the  $^{137}\text{Cs}$  profile is compatible with the bomb fallout chronology, possibly followed by a terrestrial (erosion-produced) component.

A mean sedimentation rate of  $0.49 \text{ cm}\cdot\text{yr}^{-1}$  was obtained from the investigated core with increasing trend towards present (Fig. 4). From 1920's to 1980's the sedimentation rate is rather constant:  $0.42 \text{ cm}\cdot\text{yr}^{-1}$ , in 1990's the rate increases to an average  $0.58 \text{ cm}\cdot\text{yr}^{-1}$  and in the 21<sup>st</sup> Century it reaches  $0.90 \text{ cm}\cdot\text{yr}^{-1}$ . Generally, a relatively increased recent sedimentation rate can be observed comparing to an average sedimentation rate at higher depths of an

associated gravity core estimated to  $0.15 \text{ cm}\cdot\text{yr}^{-1}$  by  $^{14}\text{C}$  chronology (S. Mulitza, unpublished data).

Based on transmission test with different absorbers it can be concluded, that efficiencies produced by LabSOCS and used for activities estimations (including self-absorption correction) can thus be successfully used for purposes of combined  $^{210}\text{Pb}$  and  $^{137}\text{Cs}$  chronology.

## REFERENCES

- Appleby P.G., Oldfield F., 1978. The calculation of Lead-210 dates assuming a constant rate of supply of unsupported  $^{210}\text{Pb}$  to the sediment. CATENA, 5, 1-8.
- Bronson F.L., 2003. Validation of the accuracy of the LabSOCS software for mathematical efficiency calibration of Ge detectors for typical laboratory samples. Journal of Radioanalytical and Nuclear Chemistry, 255, 1: 137-141.
- Cutshall N. H., Larsen I. L., Olsen C.R., 1983. Direct analysis of  $^{210}\text{Pb}$  in sediment samples: self-absorption corrections. Nuclear Instruments and Methods 206, 309-312.
- García-Tavalera M., Peña V., 2004. A hybrid method to compute accurate efficiencies for volume samples in  $\gamma$ -ray spectrometry. Applied Radiation and Isotopes 60, 227-232.
- Hurtado S., Villa M., Manjón G., García-Tenorino R., 2007. A self-sufficient and general method for self-absorption correction in gamma-ray spectroscopy using GEANT4. Nuclear Instruments and Methods in Physics Research A, 580,1: 234-237.
- San Miguel E. G., Pérez-Moreno J. P., Polívar J. P., García-Tenorino R., Martin J. E., 2002.  $^{210}\text{Pb}$  determination by gamma spectrometry in voluminal samples (cylindrical geometry). Nuclear Instruments and Methods in Physics Research A 493, 111-120.
- Sima O., Dovlete C., 1997. Matrix Effects in the Activity Measurement of Environmental Samples Implementation of Specific Corrections in a Gamma-ray Spectrometry Analysis Program. Applied Radiation and Isotopes 48, 59-69.
- UNSCEAR, 2000. Sources and Effects of Ionizing Radiation: United Nations Scientific Committee on the Effects of Atomic Radiation UNSCEAR 2000 Report to the General Assembly, with Scientific Annexes. Annex C: Exposures to the Public from Man-made Sources of Radiation. United Nations, New York.